

Determination of Trace Lead, Cadmium, and Arsenic (III) in Municipal Wastewater by Anodic Stripping Voltammetry

Shengcun Ma, Guo Zhao, Xingyu Chen, Ashok Mulchandani*, David Jassby**

July 10, 2020

•• **UCLA** ••

•• **UCR** ••


Water-Energy Nexus

- 83% of electricity in the USA is produced by thermoelectric power plants.

- Fossil-fuel power plant
- Nuclear power plant

- Water is a critical component of thermoelectrical plants


- Electricity generation
- Cooling

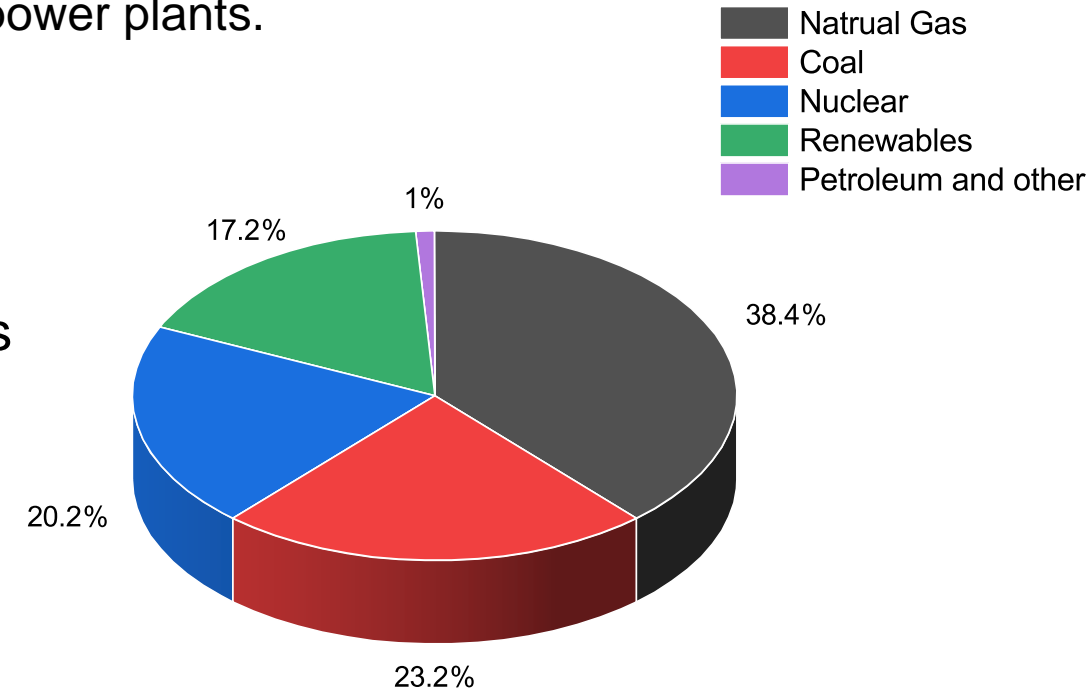

U.S. Electricity generation by major energy source
(2019)

Alternative Water Resource

- Water scarcity
 - Related to Climate change
 - Caused a drop in electricity production
- Municipal wastewater water (MWW)
 - Widespread availability
 - Relatively uniform quality

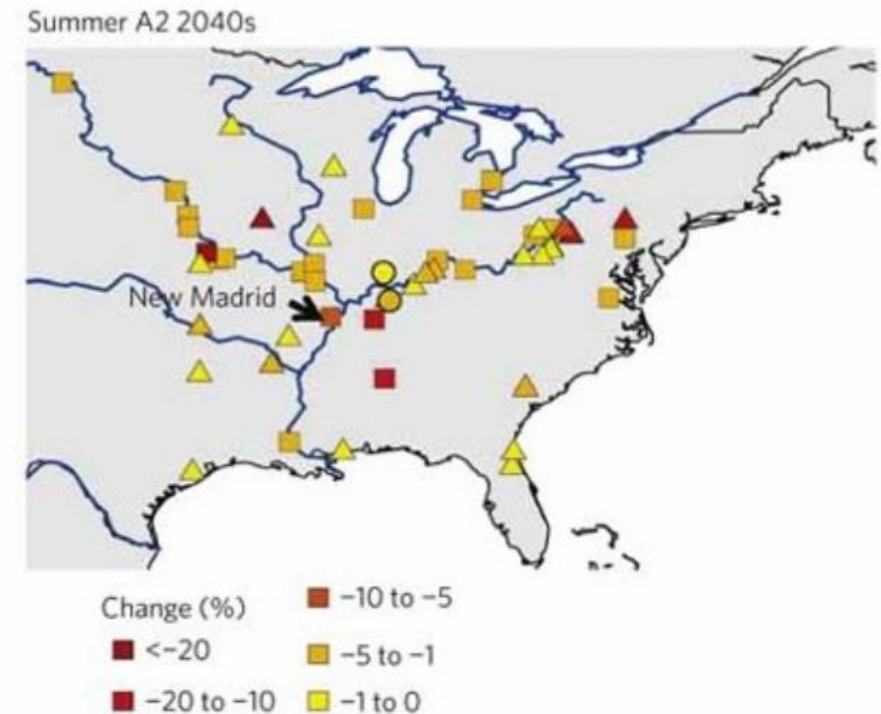


Projected decreased water resources for thermoelectrical plants

Challenges with MWW

- Metal Pollutions in Cooling water
 - Metals introduced from pipe corrosion
 - Metals existing in MWW

There is a strong imperative to frequently monitor heavy metals.

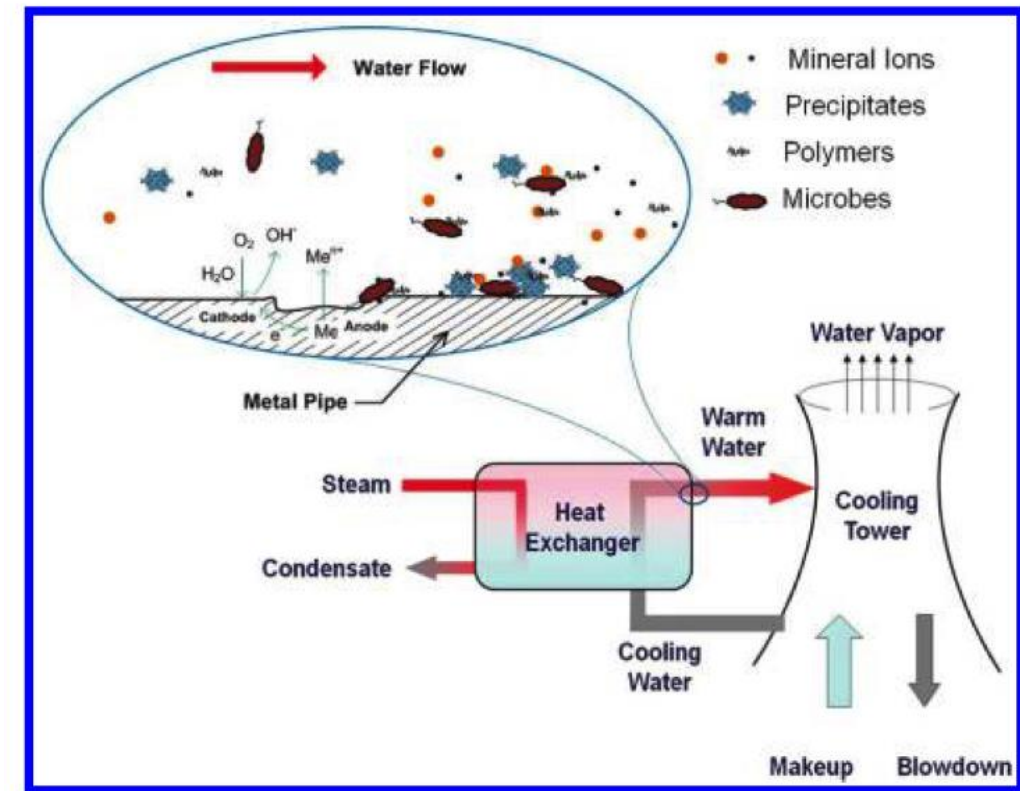

Metal pollutions introduced from the pipes

Challenges with Metal Detection

- Limitations of mature metal detection techniques
 - Expensive
 - Dedicated staff required
 - Grab-sampling required
 - Lengthy processing

The device that could autonomously conduct metal measurements is desirable.




Anodic Stripping Voltammetry (ASV)

Advantages

- Low-cost
- High sensitivity
- Easy to be miniaturized
- Easy to be automated

Limitation

- Only ionic metals are ready for ASV detections

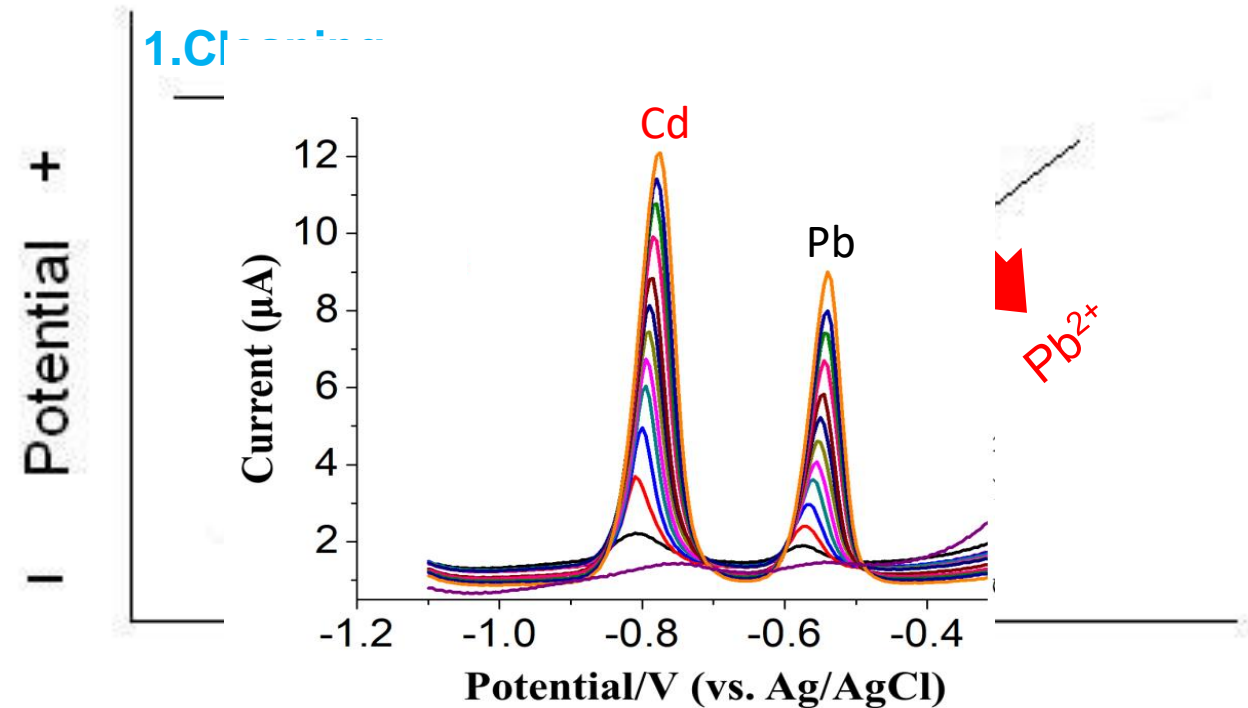

Metals in MWW


- Complex with natural organic substances
- Bind with inorganic substances
- Absorbed by various components

Important to develop pre-treatment methods which could release metal ions

Large organic or inorganic substance



Small organic molecules

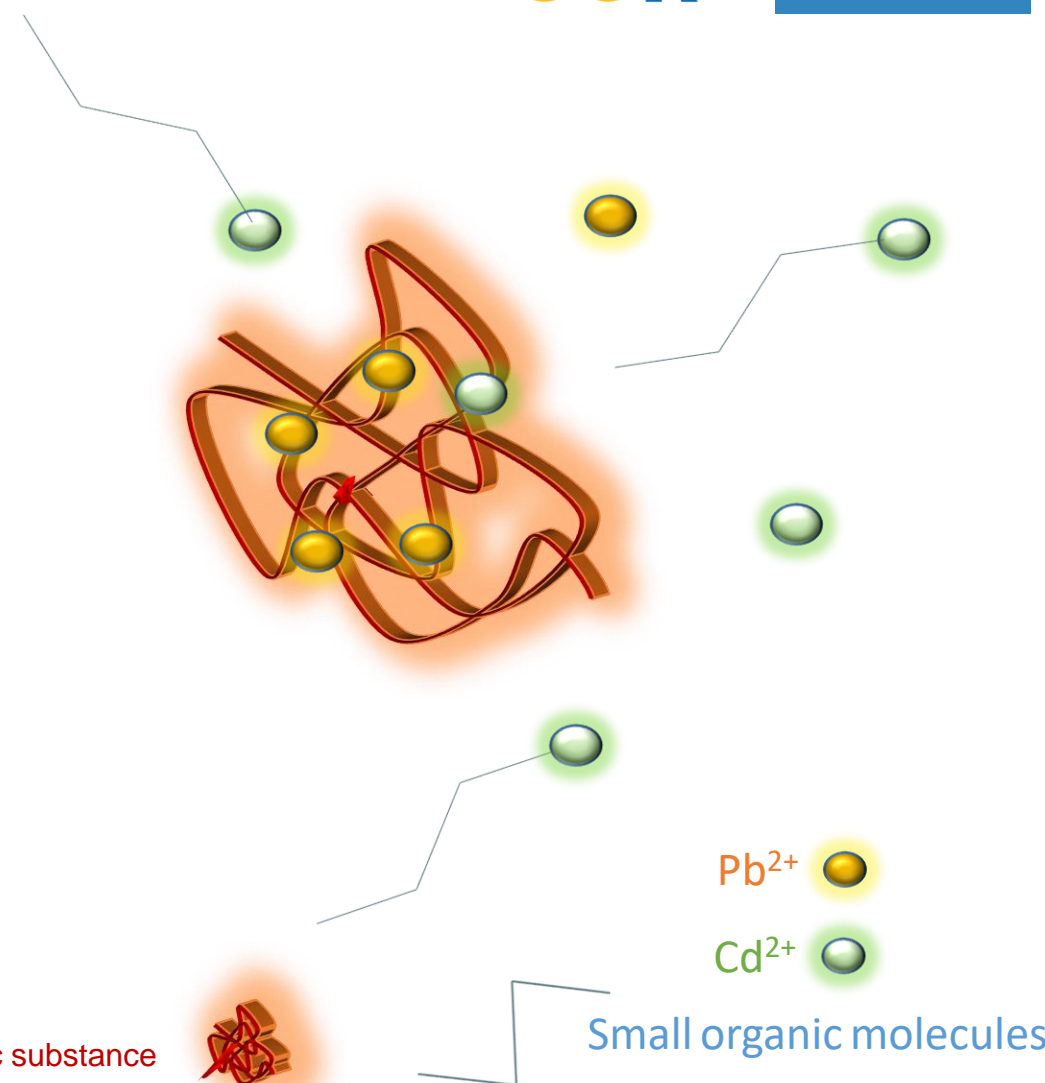

Methods

- Electrode synthesis
- Pretreatment Method Investigations

Electrode Fabrication

- Arsenic detection
 - Au-Fe₃O₄ modified glassy carbon electrode (GCE)
 - Increase conductivity and arsenic sorption ability
- Pb and Cd detection
 - (BiO)₂CO₃-rGO-Nafion modified GCE
 - (BiO)₂CO₃ facilitates the preconcentration of Pb and Cd
 - rGO increases the conductivity
 - Nafion enhances structural stability



Composite material modified GCE





GCE



Au-Fe₃O₄ nano particles

Pretreatment

- Acidification
 - Dissolve inorganic substances
 - Precipitate humic acid
- Ultraviolet (UV)/H₂O₂
 - Produce hydroxyl radicals (*OH)

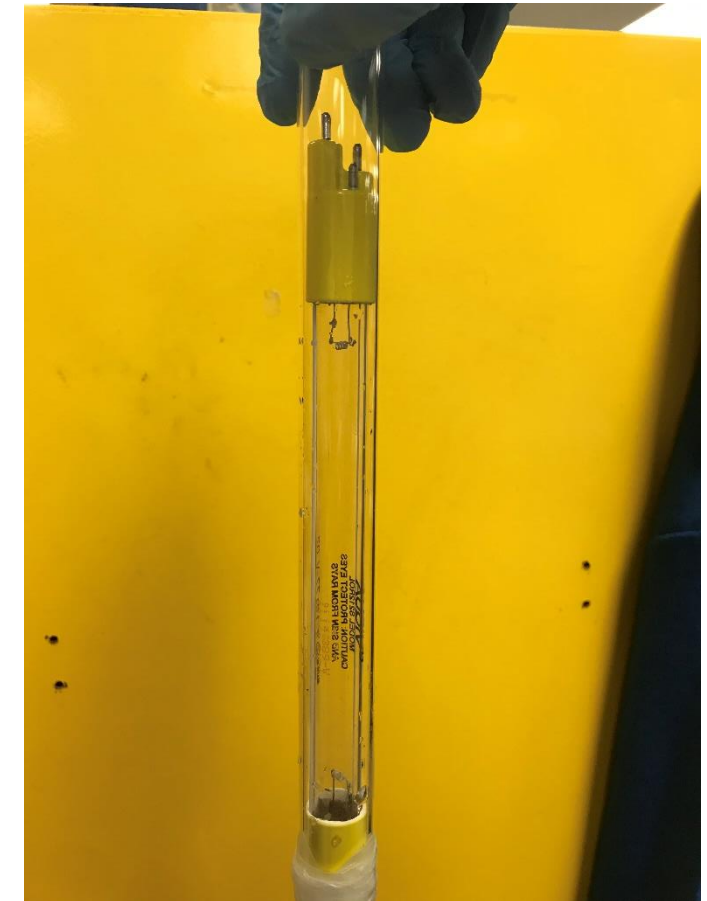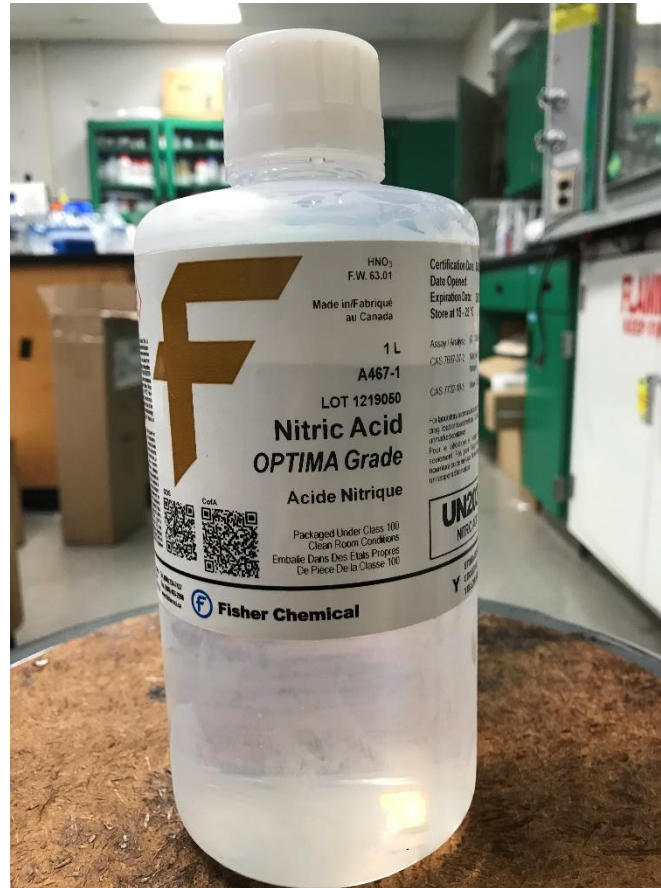


Results & Discussion

- Performances of electrode
- Automation

ASV Performances in DI water


- The response peaks increased linearly with increasing concentrations, with well-defined stripping peaks observed.
- The limit of detection is very low (i.e., we could achieve a high sensitivity)
 - Pb: 0.24 ppb << (Discharge limit: 2.5 ppb)
 - Cd: 0.16 ppb << (Discharge limit: 0.7 ppb)
 - As: 0.22 ppb << (Discharge limit: 150 ppb)

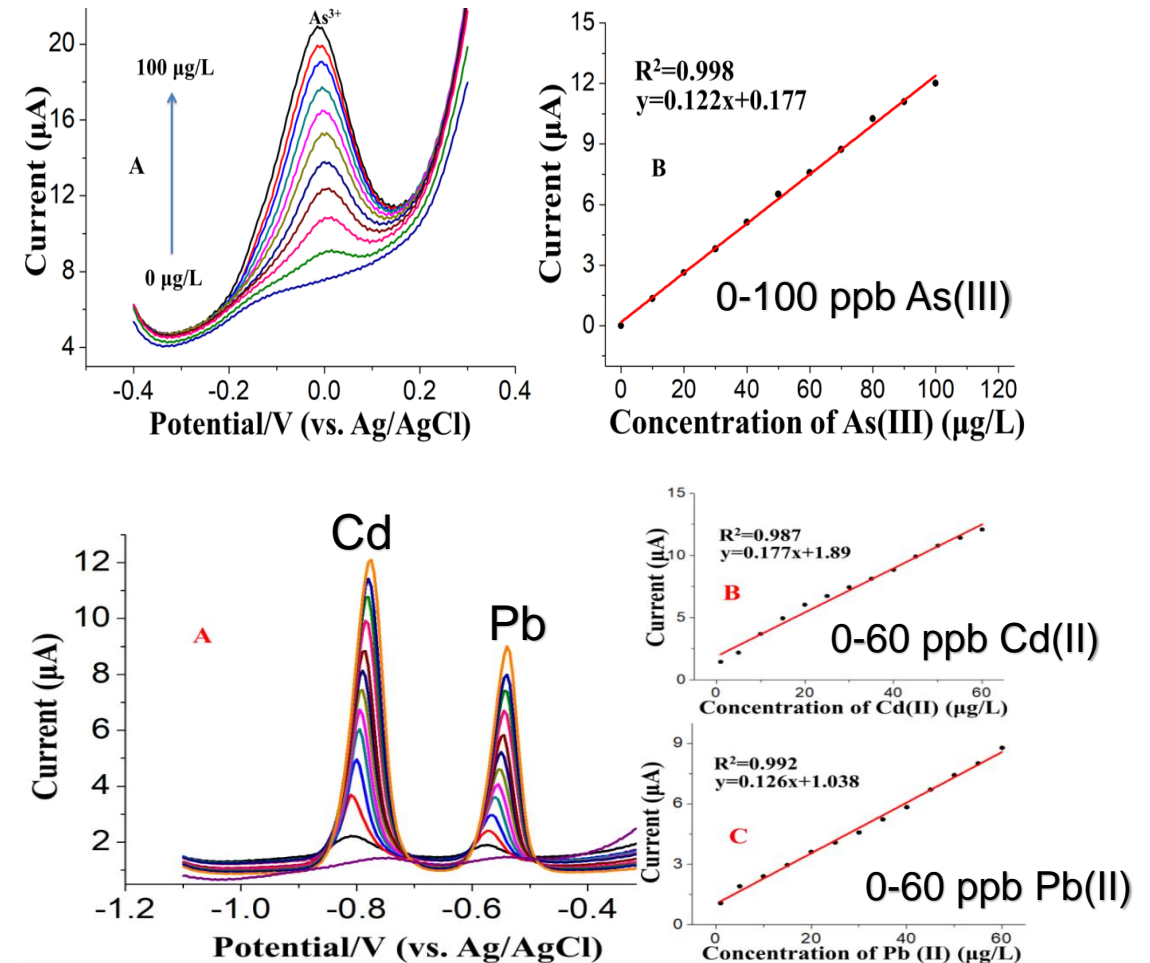

ASV Performances in MWW

As detections


- ASV could directly detect ~900 ppb As(III) in MWW without any pretreatment
 - As(III) has a high pKa (9.23), which makes it very mobile.

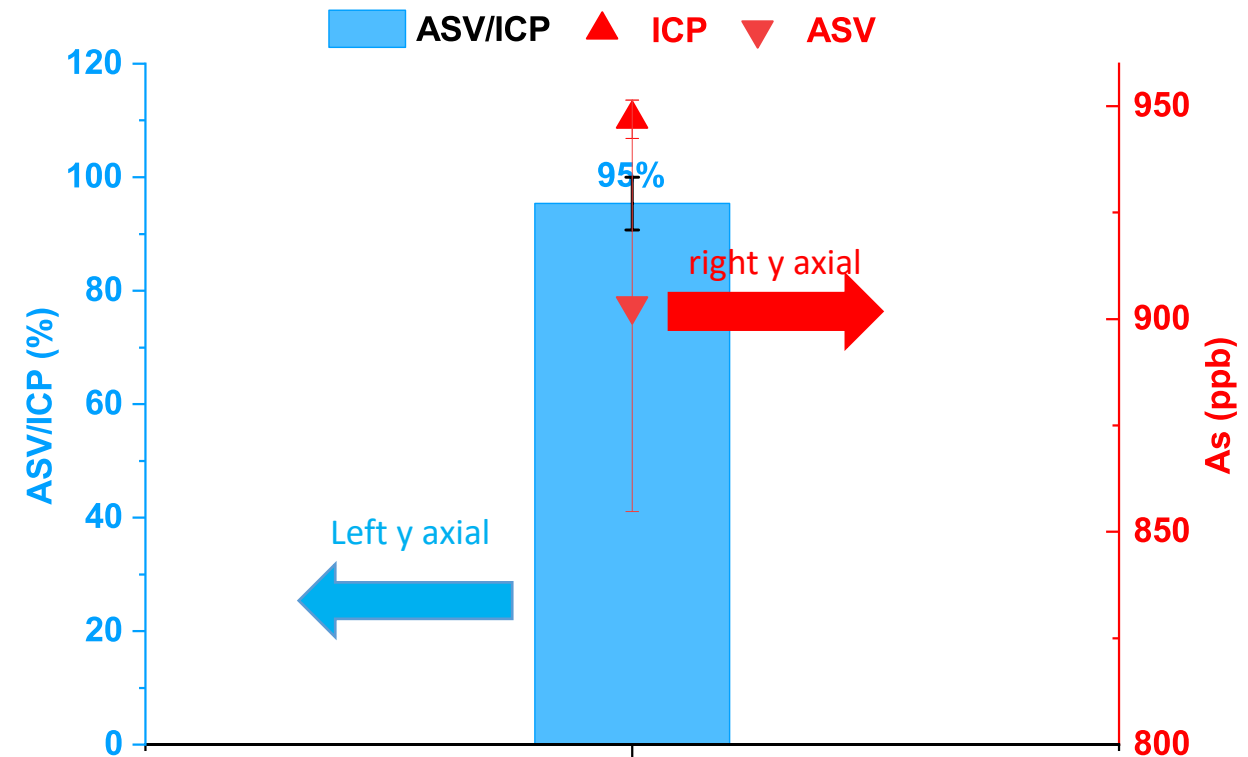

ASV Performances in MWW

Acidification for Pb detections


- Acidification treatment enabled 12.5 ppb Pb in MWW detected by ASV, while acidification

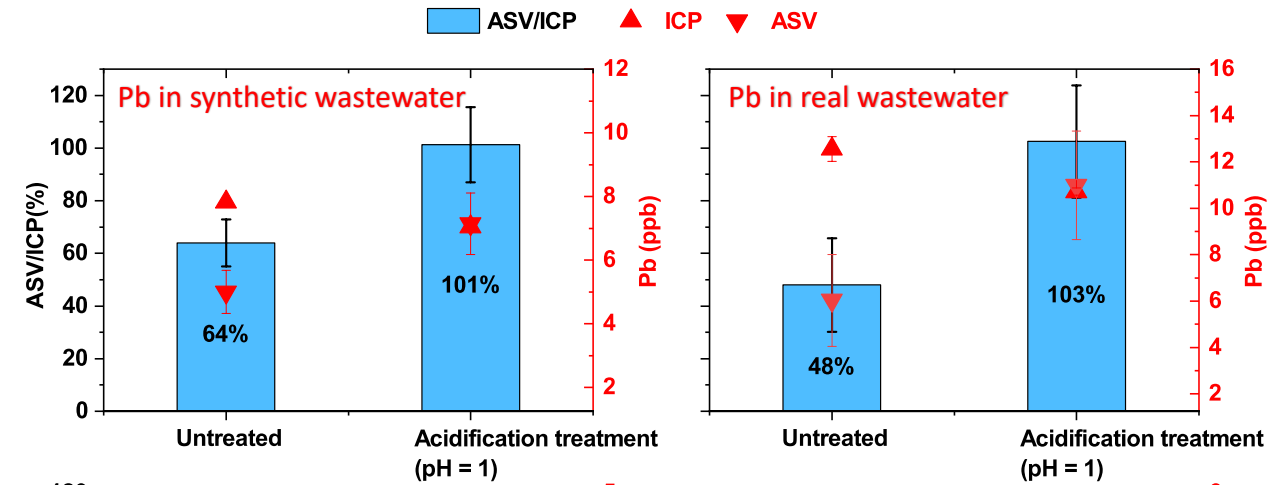


ASV Performances in MWW

UV/H₂O₂ for Cd detection


- UV/H₂O₂ treatment made ASV successfully detect most of 3.5 ppb Pb, while it failed to make 12.5 ppb Cd detectable.

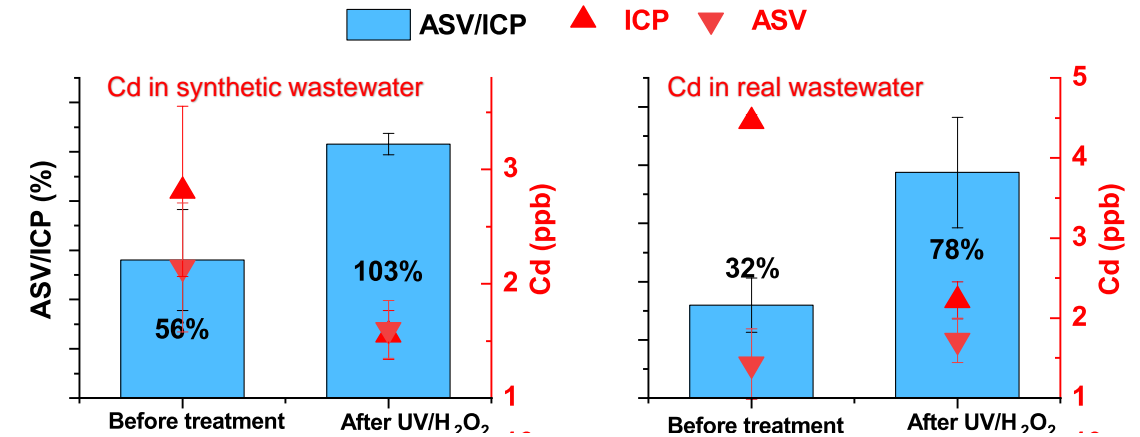

Automation

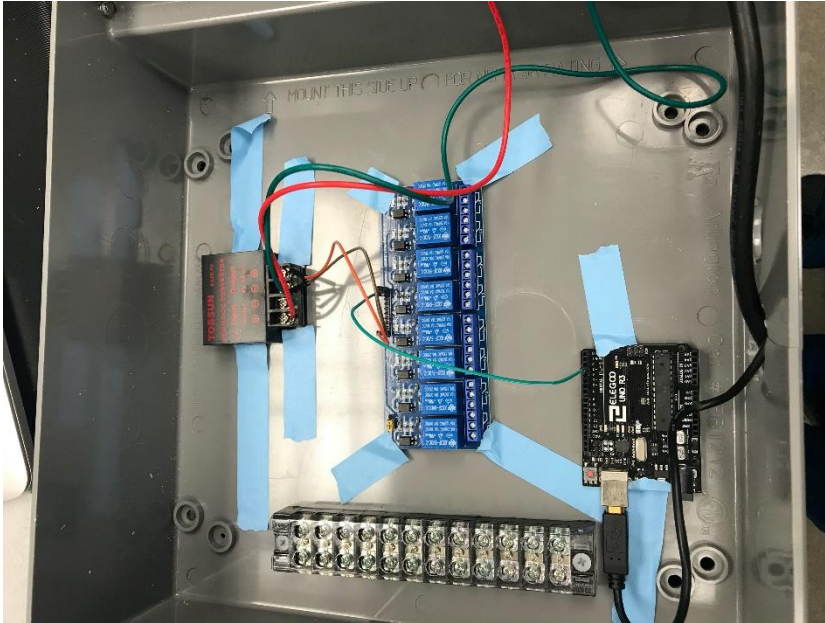

Arduino-based hardware

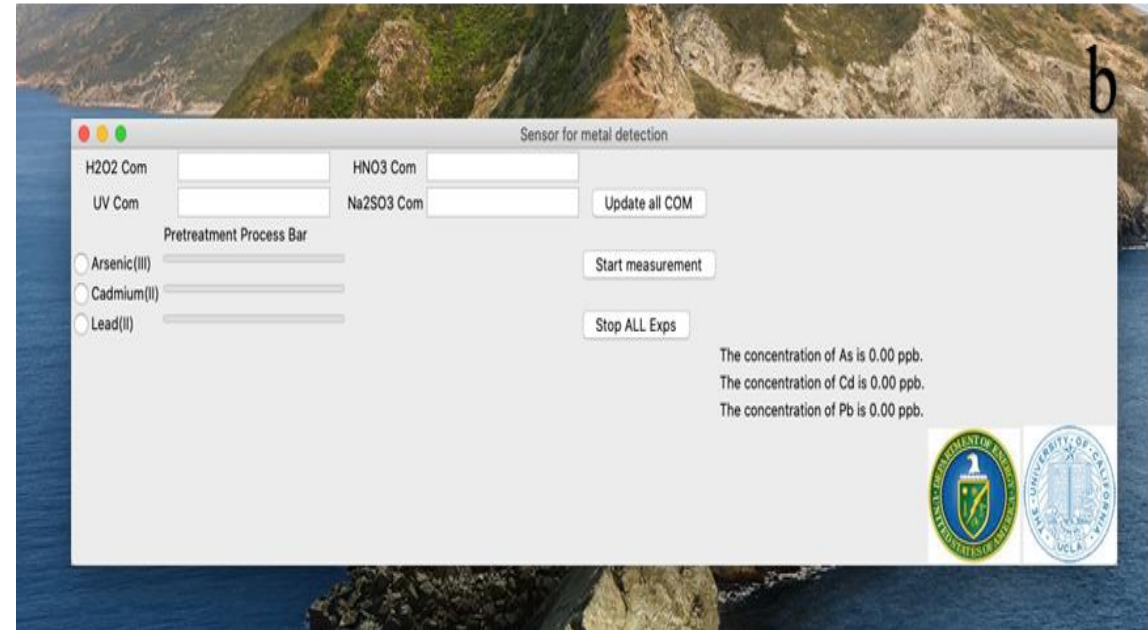

Python-based software

Conclusions

1. Our nano-material based ASV methods successfully detected all trace As(III) (i.e., ~900 ppb) in wastewater without pretreatment.
2. Acidification (i.e., adjust pH to 1) pre-treatment methods enabled the detection of trace Pb (~12.5 ppb) by ASV in wastewater.
3. A UV/H₂O₂ pre-treatment process enabled the detection of trace Cd (~3.5 ppb) by ASV in synthetic wastewater. However, ASV only measured 78% of Cd in real wastewater, and a systematic error was observed. We will solve it via using glass reactors.
4. The whole process could be automated by integration of open-source software (Python) and open-source hardware (Arduino).

Acknowledgements

- Advisor: Prof. David Jassby

Prof. Ashok Mulchandani

- Funding sources:



- Lab members



Thank You

Questions?

Shengcun Ma (shengcun@ucla.edu)

David Jassby (jassby@ucla.edu)

Ashok Mulchandani (ashok.mulchandani@ucr.edu)